

# *PRODUCT INFORMATION AND MANUAL*

## ***Human MMP-3 Instant ELISA***

### ***BMS2014INST***

Enzyme-linked immunosorbent assay for quantitative  
detection of human MMP-3.

For research use only.

Not for diagnostic or therapeutic procedures.

128 Tests

**Human MMP-3  
BMS2014INST**



Bender MedSystems GmbH  
Campus Vienna Biocenter 2  
A-1030 Vienna, Austria, Europe

## TABLE OF CONTENTS

1	Intended Use	3
2	Summary	3
3	Principles of the Test	4
4	Reagents Provided	5
5	Storage Instructions	6
6	Specimen Collection	6
7	Materials Required But Not Provided	7
8	Precautions for Use	8
9	Preparation of Reagents and Samples	10
10	Test Protocol	11
11	Calculation of Results	15
12	Limitations	19
13	Performance Characteristics	20
14	Bibliography	25
15	Ordering Information	27
16	Reagent Preparation Summary	28
17	Test Protocol Summary	29

## 1 Intended Use

The human MMP-3 Instant ELISA is an enzyme-linked immunosorbent assay for the quantitative detection of human MMP-3. **The human MMP-3 Instant ELISA is for research use only. Not for diagnostic or therapeutic procedures**

## 2 Summary

The matrix metalloproteinases (MMPs) represent a family of more than 15 Zn-dependent endopeptidases with extracellular activity. They share a common conserved protease domain sequence in which three His residues form a complex with a catalytic Zn ion. Further, all MMPs contain a regulatory domain with a conserved motif.

The family of MMPs are capable of breaking down any extracellular matrix component. In normal physiology, MMPs produced by connective tissue are thought to contribute to tissue remodeling in development, in the menstrual cycle and in repair processes following tissue damage. In pathological situations mainly the involvement of breakdown of the connective tissues like in rheumatoid arthritis, cancer and periodontal and cardiovascular diseases are described. Leukocytes, mainly macrophages, are the major sources of MMP production which allow leukocytes to extravasate and penetrate tissues, which is a key event in inflammatory diseases. In parallel, metastatic cancer cells use MMPs to migrate to foreign tissue.

MMP-3, also known as Stromelysin-1, or Transin is expressed by a variety of cells including fibroblasts, endothelial cells, macrophages, osteoblasts and more. Expression is upregulated upon activation by inducers like inflammatory cytokines such as IL-1 and TNF $\alpha$ , growth factors and oncogenic transformation factors.

MMP-3 is secreted as a proenzyme stimulating plasminogen activation. Activation through cleavage of the pro-domain can be achieved by various proteases including MMP-3 itself.

The active enzyme consists of defined domains like the zinc-binding motif and the regulatory hemopexin-like domain. A large number of proteins have been shown to act as substrates for MMP-3, most important collagens III, IV, V and X, gelatin, aggrecan, fibronectin, laminin, elastin, casein, Substance P, IL-1 $\beta$ , serum amyloid A, IGFBP-3 and the MMPs -1, 7, 8, 9 and 13. Therefore MMP-3 plays an important role in matrix turnover and pathological destruction of the tissue.

### 3 Principles of the Test

An anti-human MMP-3 coating antibody is adsorbed onto microwells. Human MMP-3 present in the sample or standard binds to antibodies adsorbed to the microwells; an anti-human MMP-3 detection antibody binds to human MMP-3 captured by the first antibody. IgG-HRP (2<sup>nd</sup> Antibody/HRP-Conjugate) binds to the anti-human MMP-3 detection antibody.

Following incubation unbound anti-human MMP-3 detection antibody and IgG-HRP is removed during a wash step, and substrate solution reactive with HRP is added to the wells.

A coloured product is formed in proportion to the amount of human MMP-3 present in the sample. The reaction is terminated by addition of acid and absorbance is measured at 450 nm. A standard curve is prepared from 7 human MMP-3 standard dilutions and human MMP-3 sample concentration determined.

Figure 1

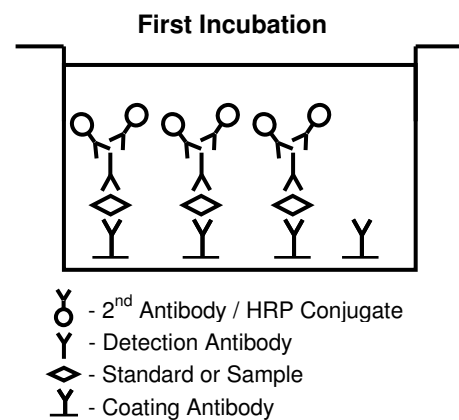


Figure 2


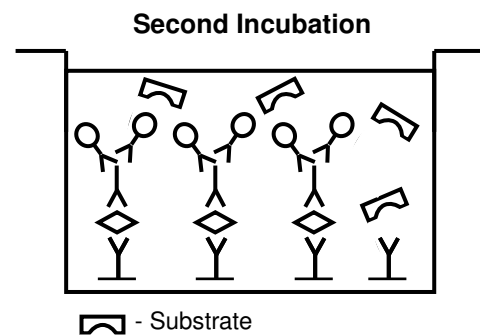


Figure 3

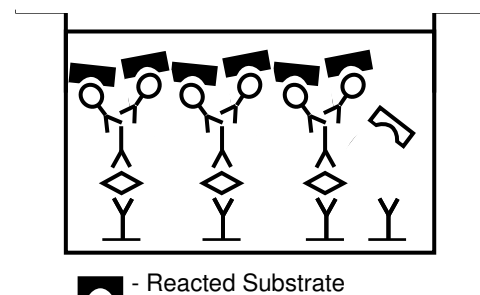

#### 4 Reagents Provided

- 1 aluminium pouch with a **Microwell Plate coated with polyclonal antibody** to human MMP-3, **Detection Antibody** (anti-human MMP-3 monoclonal antibody), **IgG-HRP** (2<sup>nd</sup> Antibody/HRP-Conjugate) and Sample Diluent, lyophilized
- 2 aluminium pouches with a human MMP-3 **Standard curve** (coloured)
- 1 bottle (25 ml) **Wash Buffer Concentrate 20x** (phosphate-buffered saline with 1% Tween 20)
- 1 vial ( 12 ml) **Sample Diluent**  
(Use when an external predilution of the samples is needed)
- 1 vial (15 ml) **Substrate Solution** (tetramethyl-benzidine)
- 1 vial (15 ml) **Stop Solution** (1M Phosphoric acid)
- 2 **Adhesive Films**

## 5 Storage Instructions

Store ELISA plate and Standard curves or whole kit at -20 °C. The plate and the standard curves can also be removed, stored at -20 °C, remaining kit reagents can be stored between 2° and 8 °C. Expiry of the kit and reagents is stated on labels.

The expiry of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, the reagent is not contaminated by the first handling.

## 6 Specimen Collection

Cell culture supernatant and serum were tested with this assay. Other biological samples might be suitable for use in the assay. Remove serum from the clot as soon as possible after clotting.

Samples containing a visible precipitate must be clarified prior to use in the assay. Do not use grossly hemolyzed or lipemic specimens.

Pay attention to a possible “**Hook Effect**” due to high sample concentrations (see chapter 11).

Samples must be stored frozen at -20 °C to avoid loss of bioactive human MMP-3. If samples are to be run within 24 hours, they may be stored at 2° to 8 °C (for sample stability refer to 13).

Avoid repeated freeze-thaw cycles. Prior to assay, the frozen sample should be brought to room temperature slowly and mixed gently.

## **7 Materials Required But Not Provided**

- 5 ml and 10 ml graduated pipettes
- 5  $\mu$ l to 1000  $\mu$ l adjustable single channel micropipettes with disposable tips
- adjustable multichannel micropipettes (for volumes between 50  $\mu$ l and 500  $\mu$ l) with disposable tips
- Multichannel micropipette reservoir
- Beakers, flasks, cylinders necessary for preparation of reagents
- Device for delivery of wash solution (multichannel wash bottle or automatic wash system)
- Microwell strip reader capable of reading at 450 nm (620 nm as optional reference wave length)
- Glass-distilled or deionized water
- Statistical calculator with program to perform linear regression analysis

## 8 Precautions for Use

- All chemicals should be considered as potentially hazardous. We therefore recommend that this product is handled only by those persons who have been trained in laboratory techniques and that it is used in accordance with the principles of good laboratory practice. Wear suitable protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken to avoid contact with skin or eyes. In the case of contact with skin or eyes wash immediately with water. See material safety data sheet(s) and/or safety statements(s) for specific advice.
- Reagents are intended for research use only and are not for use in diagnostic or therapeutic procedures.
- Do not mix or substitute reagents with those from other lots or other sources.
- Do not use kit reagents beyond expiration date on label.
- Do not expose kit reagents to strong light during storage or incubation.
- Do not pipette by mouth.
- Do not eat or smoke in areas where kit reagents or samples are handled.
- Avoid contact of skin or mucous membranes with kit reagents or specimens.
- Rubber or disposable latex gloves should be worn while handling kit reagents or specimens.
- Avoid contact of substrate solution with oxidizing agents and metal.
- Avoid splashing or generation of aerosols.
- In order to avoid microbial contamination or cross-contamination of reagents or specimens which may invalidate the test use disposable pipette tips and/or pipettes.
- Use clean, dedicated reagent trays for dispensing substrate reagent.

- Glass-distilled water or deionized water must be used for reagent preparation.
- Substrate solution must be at room temperature prior to use.
- Decontaminate and dispose specimens and all potentially contaminated materials as they could contain infectious agents. The preferred method of decontamination is autoclaving for a minimum of 1 hour at 121.5°C.
- Liquid wastes not containing acid and neutralized waste may be mixed with sodium hypochlorite in volumes such that the final mixture contains 1.0% sodium hypochlorite. Allow 30 minutes for effective decontamination. Liquid waste containing acid must be neutralized prior to the addition of sodium hypochlorite.

## 9 Preparation of Reagents and Samples

**Buffer concentrate** should be brought to room temperature and diluted before starting the test procedure. If crystals have formed in the **buffer concentrate**, warm it gently until crystals have completely dissolved.

### 9.1 Wash Buffer (1x)

Pour entire contents (25 ml) of the Wash Buffer Concentrate (20x) into a clean 500 ml graduated cylinder. Bring to final volume to 500 ml with glass-distilled or deionized water. Mix gently to avoid foaming. The pH of the final solution should adjust to 7.4.

Transfer to a clean wash bottle and store at 2° to 25°C. Please note that Wash Buffer (1x) is stable for 30 days.

## 10 Test Protocol

- **Use plate immediately after removal from -20 °C!**
  - **Do not wait until pellets have completely dissolved before applying samples - the binding reaction in the standard strips starts immediately after addition of water!**
  - **Do not try to dissolve pellets by pipetting up and down in the wells - some parts of the pellet could stick to the tip creating high variation of results.**
  - **Perform the washing step with at least 400 µl of washing buffer as stated in the manual or fill the wells completely - otherwise any pellet residues sticking to the rim of the well will not be removed and create high variation of results.**
  - **Allow the washing buffer to sit in the wells for a few seconds before aspiration.**
  - **Remove covers of the standard strips carefully so that all the lyophilized pellets remain in the wells.**
- a. Determine the number of Microwell Strips required to test the desired number of samples plus Microwell Strips for blanks and standards (coloured). Each sample, standard and blank should be assayed in duplicate. Remove extra Microwell Strips from holder and store in foil bag with the desiccant provided at -20 °C sealed tightly. Place Microwell Strips containing the standard curve in position A1/A2 to H1/H2 (see Table 1).
  - b. Add 130 µl of **distilled water** to the **sample wells**.
  - c. Add **distilled water** to all **standard and blank wells** as indicated on the label of the standard strips (A1, A2 to H1, H2).

Table 1

Table depicting an example of the arrangement of blanks, standards and samples in the microwell strips:

	<b>1</b>	<b>2</b>	<b>3</b>	<b>4</b>
<b>A</b>	Standard 1 (50 ng/ml)	Standard 1 (50 ng/ml)	Sample 1	Sample 1
<b>B</b>	Standard 2 (25 ng/ml)	Standard 2 (25 ng/ml)	Sample 2	Sample 2
<b>C</b>	Standard 3 (12.5 ng/ml)	Standard 3 (12.5 ng/ml)	Sample 3	Sample 3
<b>D</b>	Standard 4 (6.25 ng/ml)	Standard 4 (6.25 ng/ml)	Sample 4	Sample 4
<b>E</b>	Standard 5 (3.13 ng/ml)	Standard 5 (3.13 ng/ml)	Sample 5	Sample 5
<b>F</b>	Standard 6 (1.56 ng/ml)	Standard 6 (1.56 ng/ml)	Sample 6	Sample 6
<b>G</b>	Standard 7 (0.78 ng/ml)	Standard 7 (0.78 ng/ml)	Sample 7	Sample 7
<b>H</b>	Blank	Blank	Sample 8	Sample 8

- d. Add 20  $\mu\text{l}$  of each **sample**, in duplicate, to the **designated wells** and mix the contents.
- e. Cover with an adhesive film and incubate at room temperature (18°C to 25°C) for 3 hours, if available on a microplate shaker at 200 rpm.
- f. Remove adhesive film and empty wells. **Wash** the microwell strips **6 times** with approximately **400  $\mu\text{l}$**  Wash Buffer per well with thorough aspiration of microwell contents between washes. Allow the Wash Buffer to sit in the wells for about **10 – 15 seconds** before aspiration. Take care not to scratch the surface of the microwells.

After the last wash, tap microwell strips on absorbent pad or paper towel to remove excess Wash Buffer. Use the microwell strips immediately after washing or place upside down on a wet absorbent paper for no longer than 15 minutes. Do not allow wells to dry.

- g. Pipette 100  $\mu\text{l}$  of **TMB Substrate Solution** to all wells, including the blank wells.
- h. Incubate the microwell strips at room temperature (18° to 25°C) for about 10 min. Avoid direct exposure to intense light.

**The colour development on the plate should be monitored and the substrate reaction stopped (see next point of this protocol) before positive wells are no longer properly recordable. Determination of the ideal time period for colour development has to be done individually for each assay.**

It is recommended to add the Stop Solution when the highest standard has developed a dark blue colour. Alternatively the colour development can be monitored by the ELISA reader at 620 nm. The substrate reaction should be stopped as soon as Standard 1 has reached an OD of 0.6 – 0.65.

- i. Stop the enzyme reaction by quickly pipetting 100  $\mu\text{l}$  of **Stop Solution** into each well, including the blank wells. It is important that the Stop Solution is spread quickly and uniformly throughout the microwells to completely inactivate the enzyme. Results must be read immediately after the Stop Solution is added or within one hour if the microwell strips are stored at 2 - 8°C in the dark.

- j. Read absorbance of each microwell on a spectro-photometer using 450 nm as the primary wave length (optionally 620 nm as the reference wave length; 610 nm to 650 nm is acceptable). Blank the plate reader according to the manufacturer's instructions by using the blank wells. Determine the absorbance of both the samples and the human MMP-3 standards.

**Note: In case of incubation without shaking the obtained O.D. values may be lower than indicated below. Nevertheless the results are still valid.**

## 11 Calculation of Results

- Calculate the average absorbance values for each set of duplicate standards and samples. Duplicates should be within 20 per cent of the mean.
- Create a standard curve by plotting the mean absorbance for each standard concentration on the ordinate against the human MMP-3 concentration on the abscissa. Draw a best fit curve through the points of the graph (a 5-parameter curve fit is recommended).
- To determine the concentration of circulating human MMP-3 for each sample, first find the mean absorbance value on the ordinate and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the abscissa and read the corresponding human MMP-3 concentration.
- **\*Samples have been diluted 1:5, thus the concentration read from the standard curve must be multiplied by the dilution factor (x 5).**
- **Calculation of samples with a concentration exceeding standard 1 may result in incorrect, low human MMP-3 levels (Hook Effect). Such samples require further external predilution according to expected human MMP-3 values with Sample Diluent in order to precisely quantitate the actual human MMP-3 level.**
- It is suggested that each testing facility establishes a control sample of known human MMP-3 concentration and runs this additional control with each assay. If the values obtained are not within the expected range of the control, the assay results may be invalid.
- A representative standard curve is shown in Figure 4. This curve cannot be used to derive test results. Every laboratory must prepare a standard curve for each group of microwell strips assayed.

\* N.B: There is a common dilution factor for samples due to the conjugate which must then be included in the calculation. The samples contribute 100  $\mu\text{l}$  to the final volume per well. These 100  $\mu\text{l}$  are composed of 80  $\mu\text{l}$  of Sample Diluent plus 20  $\mu\text{l}$  of the sample. This is a 1:5 dilution.

The remaining 50  $\mu\text{l}$  to give 150  $\mu\text{l}$  are due to the addition of 50  $\mu\text{l}$  conjugate to all wells.

80  $\mu\text{l}$  Sample Diluent and 50  $\mu\text{l}$  conjugate results in 130  $\mu\text{l}$  reconstitution volume, addition of 20  $\mu\text{l}$  sample (20  $\mu\text{l}$  + 80  $\mu\text{l}$  = 1:5 dilution)

Figure 4

Representative standard curve for human MMP-3 Instant ELISA. Human MMP-3 was diluted in serial 2-fold steps in Sample Diluent. Each symbol represents the mean of 3 parallel titrations.

Do not use this standard curve to derive test results. A standard curve must be run for each group of microwell strips assayed.

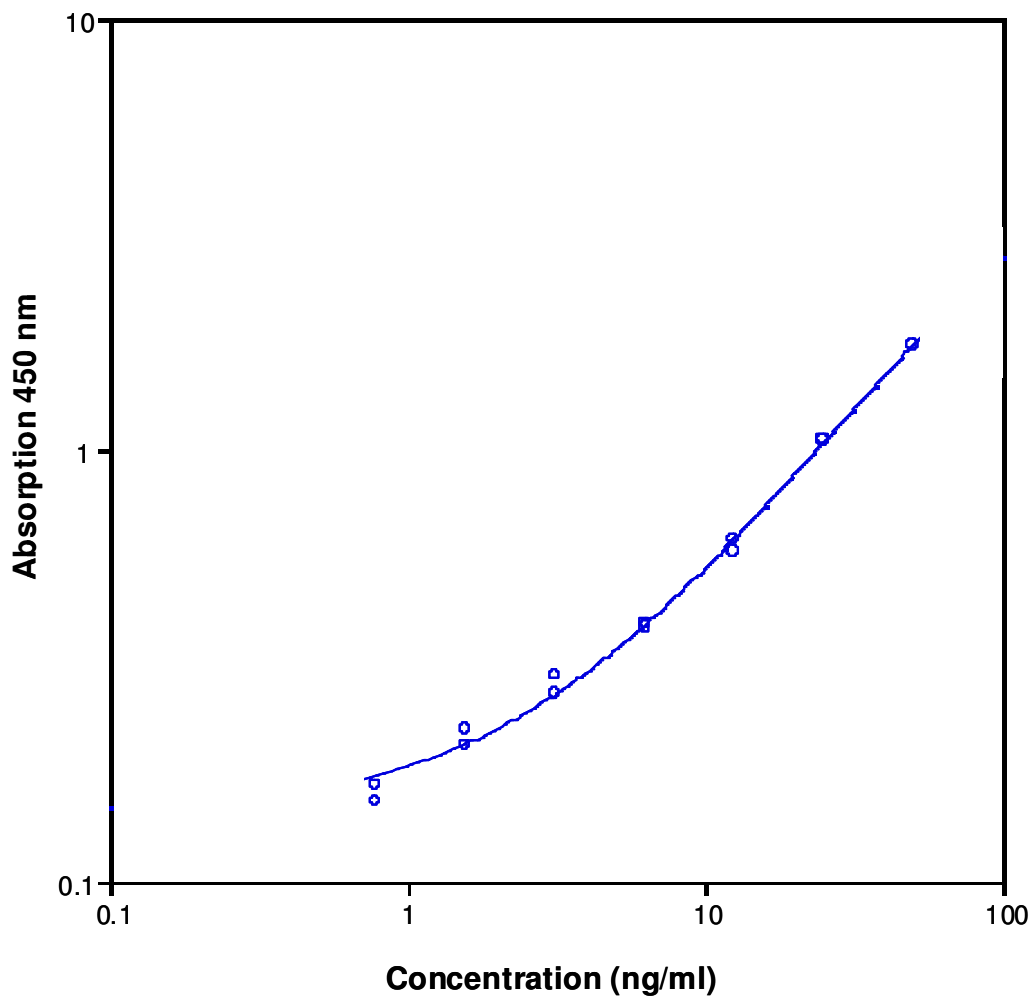


Table 2

## Typical data using the human MMP-3 INSTANT ELISA

Measuring wavelength: 450 nm

Reference wavelength: 620 nm

Standard	human MMP-3 Concentration (ng/ml)	O.D. (450 nm)	O.D. Mean	C.V. (%)
1	50.00	1.745	1.751	0.5
	50.00	1.757		
2	25.00	1.055	1.053	0.3
	25.00	1.050		
3	12.50	0.582	0.603	4.9
	12.50	0.624		
4	6.25	0.398	0.394	1.6
	6.25	0.389		
5	3.13	0.299	0.286	6.4
	3.13	0.273		
6	1.56	0.207	0.217	6.2
	1.56	0.226		
7	0.78	0.153	0.160	6.2
	0.78	0.167		
Blank	0	0.102	0.104	2.0
	0	0.105		

The OD values of the standard curve may vary according to the conditions of assay performance (e.g. operator, pipetting technique, washing technique or temperature effects). Furthermore shelf life of the kit may affect enzymatic activity and thus colour intensity. Values measured are still valid.

## 12 Limitations

- Since exact conditions may vary from assay to assay, a standard curve must be established for every run.
- Bacterial or fungal contamination of either screen samples or reagents or cross-contamination between reagents may cause erroneous results.
- Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.
- Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Empty wells completely before dispensing fresh wash solution, fill with Wash Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.
- The use of radioimmunotherapy has significantly increased the number of patients with human anti-mouse IgG antibodies (HAMA). HAMA may interfere with assays utilizing murine monoclonal antibodies leading to both false positive and false negative results. Serum samples containing antibodies to murine immunoglobulins can still be analysed in such assays when murine immunoglobulins (serum, ascitic fluid, or monoclonal antibodies of irrelevant specificity) are added to the sample.

## **13 Performance Characteristics**

### **13.1 Sensitivity**

The limit of detection of human MMP-3 defined as the analyte concentration resulting in an absorbance significantly higher than that of the dilution medium (mean plus 2 standard deviations) was determined to be 0.3 ng/ml (mean of 6 independent assays).

### **13.2 Reproducibility**

#### **13.2.1 Intra-assay**

Reproducibility within the assay was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 8 serum samples containing different concentrations of human MMP-3. 2 standard curves were run on each plate. Data below show the mean human MMP-3 concentration and the coefficient of variation for each sample (see Table 3). The calculated overall intra-assay coefficient of variation was 7.3%.

Table 3

The mean human MMP-3 concentration and the coefficient of variation for each sample.

Positive Sample	Experiment	human MMP-3 Concentration (ng/ml)	Coefficient of Variation (%)
1	1	69,9	5
	2	77.1	9
	3	81.0	7
2	1	82.4	3
	2	89.6	9
	3	101.2	6
3	1	40.9	9
	2	49.7	10
	3	46.1	6
4	1	9.5	5
	2	12.2	9
	3	11.9	9
5	1	36.3	8
	2	32.5	10
	3	31.5	5
6	1	52.6	9
	2	59.7	6
	3	60.3	5
7	1	49.0	6
	2	43.3	6
	3	54.3	8
8	1	61.9	10
	2	57.5	8
	3	61.5	9

### 13.2.2 Inter-assay

Assay to assay reproducibility within one laboratory was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 8 serum samples containing different concentrations of human MMP-3. 2 standard curves were run on each plate. Data below show the mean human MMP-3 concentration and the coefficient of variation calculated on 18 determinations of each sample (see Table 4). The calculated overall inter-assay coefficient of variation was 8.8%.

Table 4

The mean human MMP-3 concentration and the coefficient of variation of each sample

Sample	Mean human MMP-3 Concentration (ng/ml)	Coefficient of Variation (%)
1	76.0	7.4
2	81.1	10.4
3	45.6	9.6
4	11.2	13.1
5	33.5	7.5
6	57.5	7.4
7	48.9	11.2
8	60.3	4.0

### 13.3 Spike Recovery

The spike recovery was evaluated by spiking 4 levels of human MMP-3 into normal human serum. Recoveries were determined in 3 independent experiments with 2 replicates each. The unspiked serum was used as blank in these experiments.

Average recovery ranged from 80% to 110% with an overall mean recovery of 90%.

### 13.4 Dilution Parallelism

4 serum samples with different levels of human MMP-3 were analysed at serial 2 fold dilutions with 4 replicates each. The recovery ranged between 91% and 114% with an overall recovery of 102% (see Table 5).

Table 5

Sample	Dilution	Mean human MMP-3 Concentration (ng/ml)		% Recovery of Exp. Val.
		Expected Value	Observed Value	
1	1:5	--	108.8	--
	1:10	54.4	54.7	100.5
	1:20	27.2	25.8	95.0
	1:40	13.6	12.9	95.2
2	1:5	--	103.0	--
	1:10	51.5	58.7	113.9
	1:20	25.8	27.5	106.8
	1:40	12.9	14.4	111.6
3	1:5	--	74.3	--
	1:10	37.1	36.2	97.4
	1:20	18.6	16.9	91.1
	1:40	9.3	9.8	105.5
4	1:5	--	51.7	--
	1:10	25.9	24.7	95.4
	1:20	12.9	12.9	100.0
	1:40	6.5	6.9	106.9

## **13.5 Sample Stability**

### **13.5.1 Freeze-Thaw Stability**

Aliquots of serum samples (unspiked or spiked) were stored at -20 °C and thawed 5 times, and the human MMP-3 levels determined. There was no significant loss of human MMP-3 immunoreactivity detected by freezing and thawing.

### **13.5.2 Storage Stability**

Aliquots of serum samples (spiked or unspiked) were stored at -20 °C, 2-8 °C, room temperature (RT) and at 37 °C, and the human MMP-3 level determined after 72 h. There was no significant loss of human MMP-3 immunoreactivity detected during storage under above conditions.

## **13.6 Specificity**

The interference of circulating factors of the immune syteme was evaluated by spiking these proteins at physiologically relevant concentrations into a human MMP-3 positive serum. There was no crossreactivity detected.

## **13.7 Expected Values**

A panel of 40 serum samples from randomly selected apparently healthy donors (males and females) was tested for human MMP-3. The detected human MMP-3 levels ranged between 11 and 165 ng/ml.

## 14 Bibliography

- 1) Arza B et al. Eur J Biochem. 2000, 267: 6378.
- 2) Beckett RP et al. Drug Development Today. 1996, 1: 16
- 3) Bode W et al. FEBS Lett. 1993, 331: 134.
- 4) Fosang AJ et al. Biochem J. 1993, 295: 273.
- 5) Fosang AJ et al. J Biol Chem. 1991, 266: 15579.
- 6) Fowlkes JL et al. J Biol Chem. 1994, 269: 25742-6.
- 7) Gomez DE et al. Eur J Cell Biol. 1997, 74: 111
- 8) Imai K et al. J Biol Chem. 1995, 270: 6691-7.
- 9) Ito A et al. J Biol Chem. 1996, 271: 14657.
- 10) Jiang W et al. FEBS Lett. 1992, 312: 110.
- 11) Knäuper V et al. Biochem J. 1993, 291: 847.
- 12) Knäuper V et al. Biochem J. 1993, 295: 581.
- 13) Knäuper V et al. J Biol Chem. 1996, 271: 1544.
- 14) Mitchell TI et al. Biochim Biophys Acta. 1993, 1156: 245.
- 15) Murphy G et al. Biochem J. 1987, 248: 265.
- 16) Murphy G et al. Biochem J. 1991, 277: 277.
- 17) Nagase H, Barrett AJ et al. eds. Acad Press, San Diego. 1998, 1172-8.
- 18) Nagase H, Woessner JF Jr. J Biol Chem. 1999, 274: 2191
- 19) Nagase H. Handbook of Proteolytic Enzymes. 1998
- 20) Nagase H. Matrix Metalloproteinases in Zinc Metalloproteases in Health and Disease. Hooper NM ed., Taylor and Francis, London. 1996
- 21) Opdenakker G, Van Damme J. Cytokine. 1992, 4:251.

- 22) Parks WC, Mecham RP. Matrix Metalloproteinases. Acad Press, San Diego. 1998.
- 23) Shapiro SD et al. J Biol Chem. 1995, 270: 6351.
- 24) Windsor LJ et al. J Biol Chem. 1993, 268: 17341.

For literature update refer to **[www.bendermedsystems.com](http://www.bendermedsystems.com)**

## 15 Ordering Information

For orders please contact:

### **Europe-Headquarters**

Bender MedSystems GmbH  
Campus Vienna Biocenter 2  
A-1030 Vienna, Austria, Europe  
phone: +43 1 796 40 40 ext. 114  
fax: +43 1 796 40 40 ext. 400  
e-mail: [order@bendermedsystems.com](mailto:order@bendermedsystems.com)

### **USA**

Bender MedSystems, Inc.  
849 Hinckley Road  
Burlingame, CA 94010, USA  
toll-free phone: +1 (866) 952 2112  
toll-free fax: +1 (877) 952 2112  
phone: +1 (650) 952 2112  
fax: +1 (650) 952 2252  
e-mail: [uscustomerserv@bendermedsystems.com](mailto:uscustomerserv@bendermedsystems.com)

For technical information please contact:

e-mail: [techserv@bendermedsystems.com](mailto:techserv@bendermedsystems.com)  
**[www.bendermedsystems.com](http://www.bendermedsystems.com)**

**Cat.No. BMS2014INST human MMP-3 INSTANT ELISA**

## 16 Reagent Preparation Summary

### 16.1 Wash Buffer (1x)

Add **Wash Buffer Concentrate** 20 x (25 ml) to 475 ml distilled water

## 17 Test Protocol Summary

- Place standard strips in position A1/A2 to H1/H2.
- Add 130  $\mu$ l distilled water to sample wells.
- Add distilled water, in duplicate, to all standard and blank wells as indicated on the label of the standard strips.
- Add 20  $\mu$ l sample to designated wells.
- Cover microwell strips and incubate 3 hours at room temperature (18° to 25 °C) if available on a microplate shaker at 200 rpm.
- Empty and wash microwell strips 6 times with 400  $\mu$ l Wash Buffer.
- Add 100  $\mu$ l of TMB Substrate Solution to all wells including blank wells.
- Incubate the microwell strips for about 10 minutes at room temperature (18° to 25 °C).
- Add 100  $\mu$ l Stop Solution to all wells including blank wells.
- Blank microwell reader and measure colour intensity at 450 nm.

**Note: Samples have been diluted 1:5, thus the concentration read from the standard curve must be multiplied by the dilution factor (x 5)**